



WHOLENESS SUPPORT UNIT VERSION 2 (WSU V2) System User Guide & Instructions



Remember always that your new Wholeness Support Unit is NOT a medical device. The usage guidance provided herein is not medical advice. The use of your Orynoco Wholeness Support Unit does not replace conventional medical treatments and/or care. The Transition State Elements (TSE) are not medicines. Our products do not diagnose, cure or treat any diseases. If you have any sort of medical or health condition you should immediately seek the help and care of a licensed doctor or health care professional.

PLACEMENT

Preparing your location space is an important part of setting up your WSU. We also highly recommended using a dowser/geomancer to test your proposed location for the presence of any geopathic stress spots which may adversely affect the balance and proper functioning of your Wholeness Support Unit. Depending on your location we may be able to recommend a qualified dowser/geomancer that's familiar with our technology and its unique requirements. We can also advise you regards finding a qualified dowser/geomancer in your area otherwise.

IMPORTANT: Please make sure that you e-sign the 'Rental Agreement' or 'Purchase & Use Agreement' that we will send you a link for shortly after you have completed your order. For purchases this will activate your hardware warranty. For both purchases and rentals it confirms to us that you have read and are aware of our information regarding your site location being properly assessed and prepared before use. We're adamant about this step because it makes a significant difference regarding the benefits you can possibly receive from using your Orynoco Wholeness Support Unit.

ASSEMBLY

Once you've taken delivery it will be time to assemble your Wholeness Support Unit using the instructions below and/or watching our short [WSU Version 2 Assembly & Setup Video](#).

CONDITIONING YOUR ENVIRONMENT

Even if you won't be starting your sessions right away, we recommend that you setup your unit as soon as your space has been prepared. This is because when your unit is setup and thus operating, a healthy and highly beneficial life force energy field will begin to permeate your entire environment. You may or may not sense its presence, but it will be there regardless building strength over time to beneficially support you even when you're not doing sessions.

PREPARING YOUR BODY PRIOR TO SESSIONS

If you are new to using a Wholeness Support Unit, please begin your process by drinking TSE charged water for 3 to 7 days prior to starting your sessions. This will help balance your body's energy fields and your mind and emotions to better prepare you

for your first sessions in the unit. This helps you to be able to receive many more of the benefits which may be available to you from your new Wholeness Support Unit. If you're renting just start drinking TSE charged water as soon as you get your unit and begin to use it.

CHARGING & USING YOUR TSE DRINKING WATER

TSE Charged Water = water informed or charged by placing a sealed vial of TSE next to or in your drinking water.

Place the tightly capped Transition State Elements (TSE) vial(s) into a glass dispenser (e.g. a Kilner 5L drinks dispenser) filled with clean water such as Volvic water or filtered tap water. Allow the vial(s) of TSE time to charge the water. This can take several hours. Your TSE Charged Water can be used after only 2 hours, but it will have a stronger charge and be more effective if it's left to charge for up to 8 hours.

Drink 30-50ml of your TSE Charged Water at least three times a day. It's quite important to drink some of your TSE water before you go to sleep each night. You can also add it to your tea and coffee if you wish. You can drink as much TSE Charged Water as you like. You can even add some to your bath, laundry and cooking too. You can also water your plants with the TSE Charged Water. Your dogs, cats and other pets will love it as well.

We recommend adding it into all of the water that you use every day so that a healthy field can more completely permeate your entire environment as much as possible.

WHOLENESS SUPPORT UNIT SESSION GUIDELINES

CAUTION: people who have a pacemaker, metal implants or metal joint replacements CANNOT use this model Orynoco Wholeness Support Unit. **Please contact us for an alternative model.**

Put on some of your favourite music, light some candles, oils or incense as you prefer. A typical session in the Wholeness Support Unit lasts 15-40 minutes. It's best to start with shorter duration sessions to begin with and work up.

Create an intention for each session and write it down on slip of paper that you keep with you during the session. Sit on a comfortable chair positioned between the 4 tripods. Remove your shoes so you can sit with your feet grounded on the floor and sit peacefully. You could even read a good book during your sessions. It's important that you relax and not stress about anything. Just let your Wholeness Support Unit do its job!

If you feel uncomfortable take a break and try again later. If you feel well and great, you can spend a longer time in the unit and repeat the session again after a few hours. Either way, it's important to do a session before you go to sleep. You may feel sleepy during or after a session, in which case just go have a good rest.

You can repeat sessions daily if you wish and you're not feeling any adverse reactions. If you are limited on time or have some mild reactions then do sessions just 3 times a week.

You can follow this preparation pattern initially for about 2-3 weeks, then review your progress. Keeping a journal of what you are experiencing can be quite helpful for the purpose of review. Keep records in your journal of how you feel each day, what's changing in you, and so forth.

Sometimes re-balancing can feel odd or uncomfortable. This is sort of like moving into a wonderful new home where you like the new space, but there's a period of dis-comfort while you're getting used to the new home space. Be patient with yourself and trust in the process.

Mankind has used natural products to maintain optimal health and vitality since time immemorial. The informational fields imparted by the Wholeness Support Unit and the Transition State Elements (TSE) are entirely natural. They may be of help to you in achieving greater energetic balance, peace and wellness to all levels of a being, be it human or animal.

Remember always that your new Wholeness Support Unit is NOT a medical device. The usage guidance provided above is not medical advice. The use of your Orynoco Wholeness Support Unit does not replace conventional medical treatments and/or care. The Transition State Elements (TSE) are not medicines. Our products do not diagnose, cure or treat any diseases. If you have any sort of medical or health condition you should immediately seek the help and care of a licensed doctor or health care professional.

» See Assembly & Setup Info & Diagrams on the Following Pages «

[Watch Assembly & Setup Video](#)

ASSEMBLY & SETUP ASSISTANCE INFO & DIAGRAMS

- Unpackage and unwrap your WSU.
- Unlatch and extend the tripod legs, then securely lock them in their extended position by firmly closing the latches once again.
- Locate the threaded screw (male) on the tripod head and the screw hole (female) on the reactor head bracket.
- Fit the two together by threading the tripod screw into the threaded hole on the reactor head bracket using the knurled knob on the tripod (as shown in 2nd image below) to turn the screw.




- Be careful to NOT overtighten the screws. They only need to be tight enough to prevent the heads from changing positions inadvertently on the tripods when moving them around. You'll want to be able to fairly easily reach over to re-position the heads slightly at different angles during use from time to time.



- Be sure to leave the protective plastic bags which are fitted over the quantum field emitters in place because the small clear perspex rectangles inside of them are highly sensitive to touch.



- Setup the tripods with their reactor heads mounted in a roughly four-square type of a pattern. You'll need enough centre space between the tripods to fit your chair, yoga mat/cushion, bed or whatever you will be sitting/lying on when using the WSU.
- Find the black dots on the acrylic protective tubes on the reactor heads and ensure they are facing each other as shown. The adjusting handles on the tripods should be facing outward as shown.

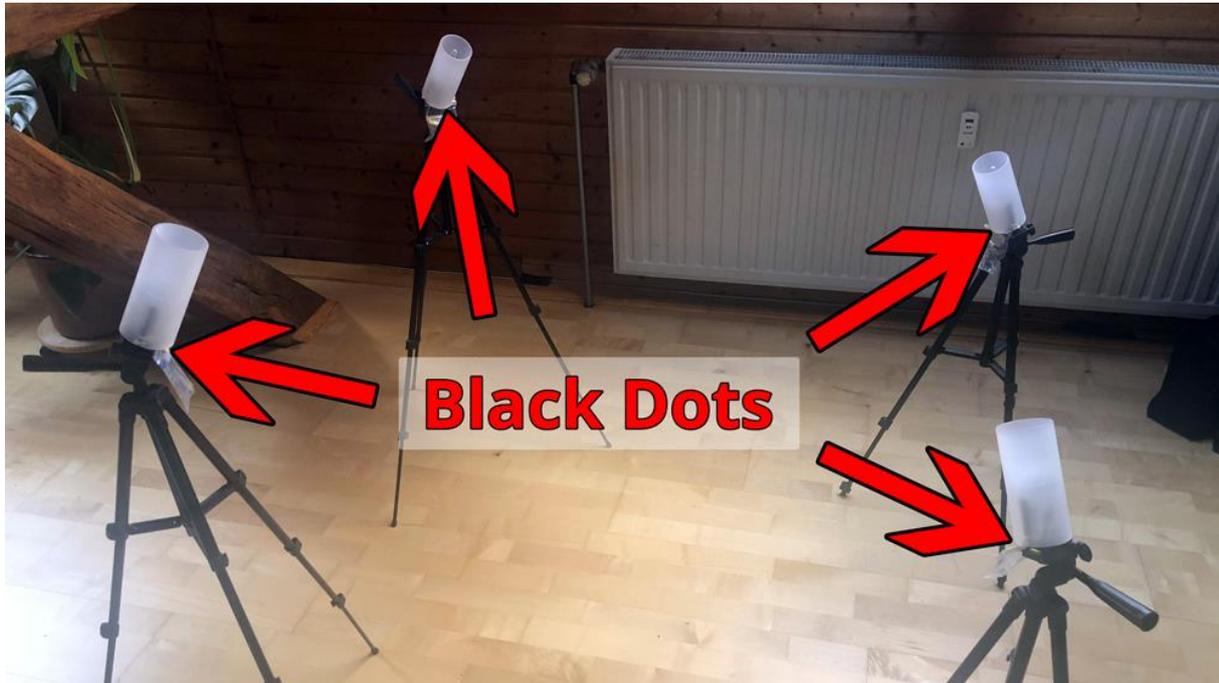

- When first starting out using the WSU, it's usually best to have ALL FOUR reactor heads pointing mostly upwards because the energy is far less intense this way.
- Once you are accustomed to the energy you can start tilting the reactor heads so they point more inwards at yourself or the person, animal or plants residing in the centre space.

